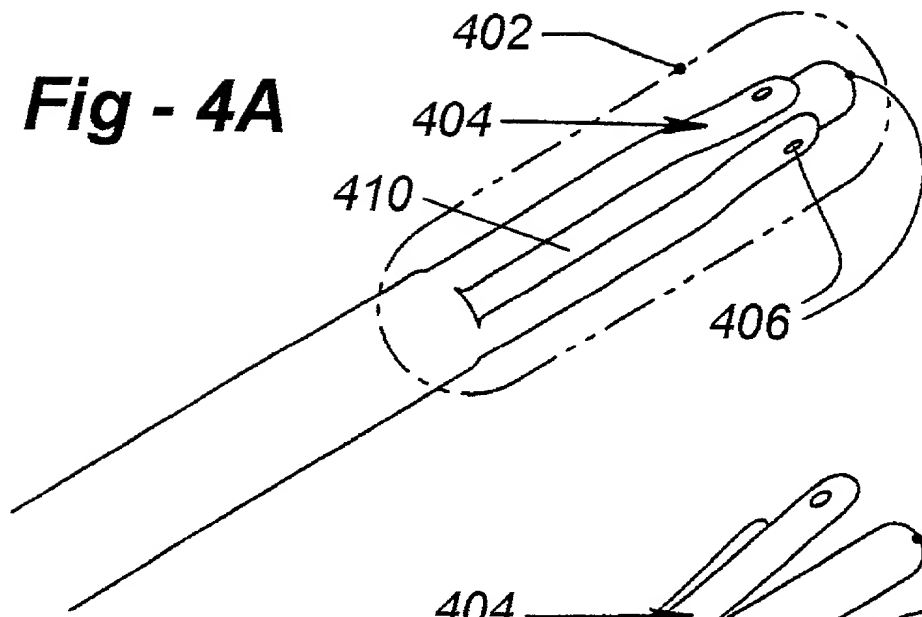
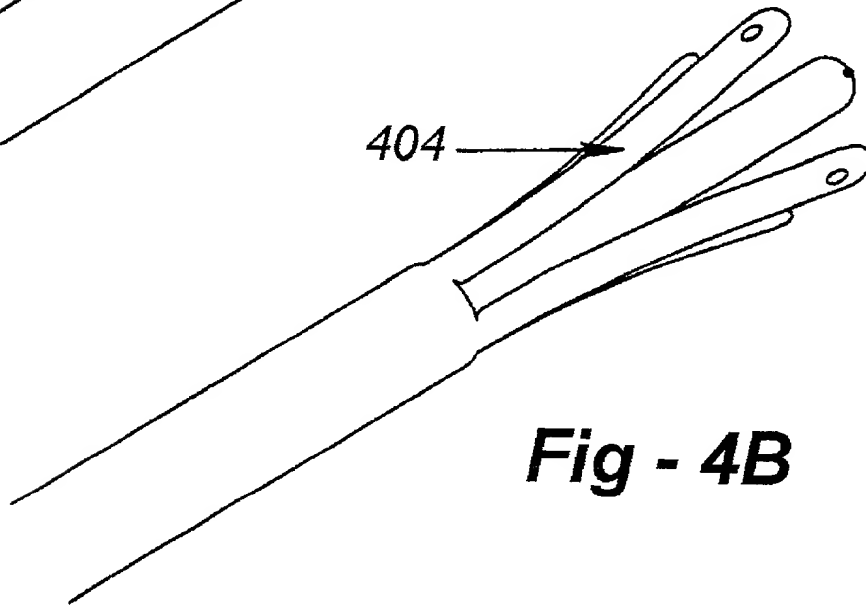



**Fig - 4A**



**Fig - 4B**



**Fig - 4D**

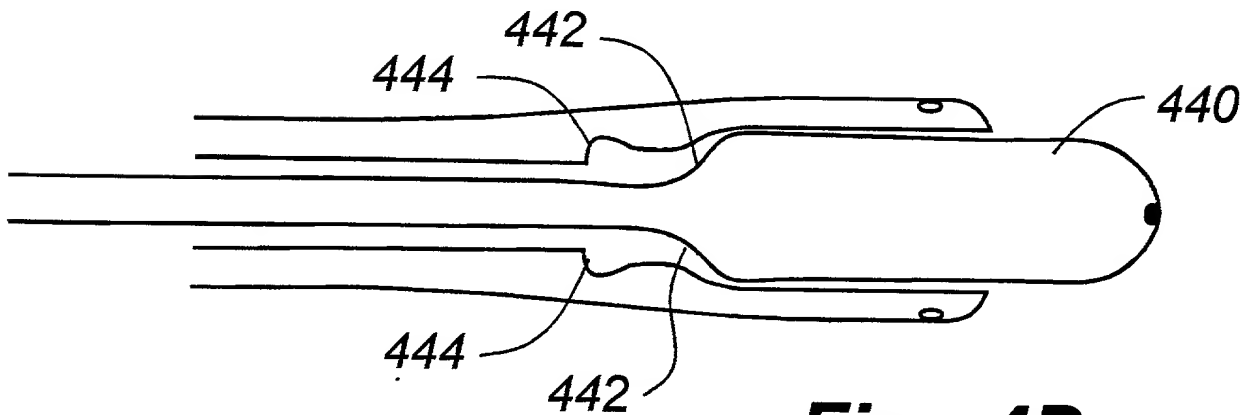

# Absolute & Percent Error for 1, 1.5, 2 mm Diameter Thermal Sensing Catheter

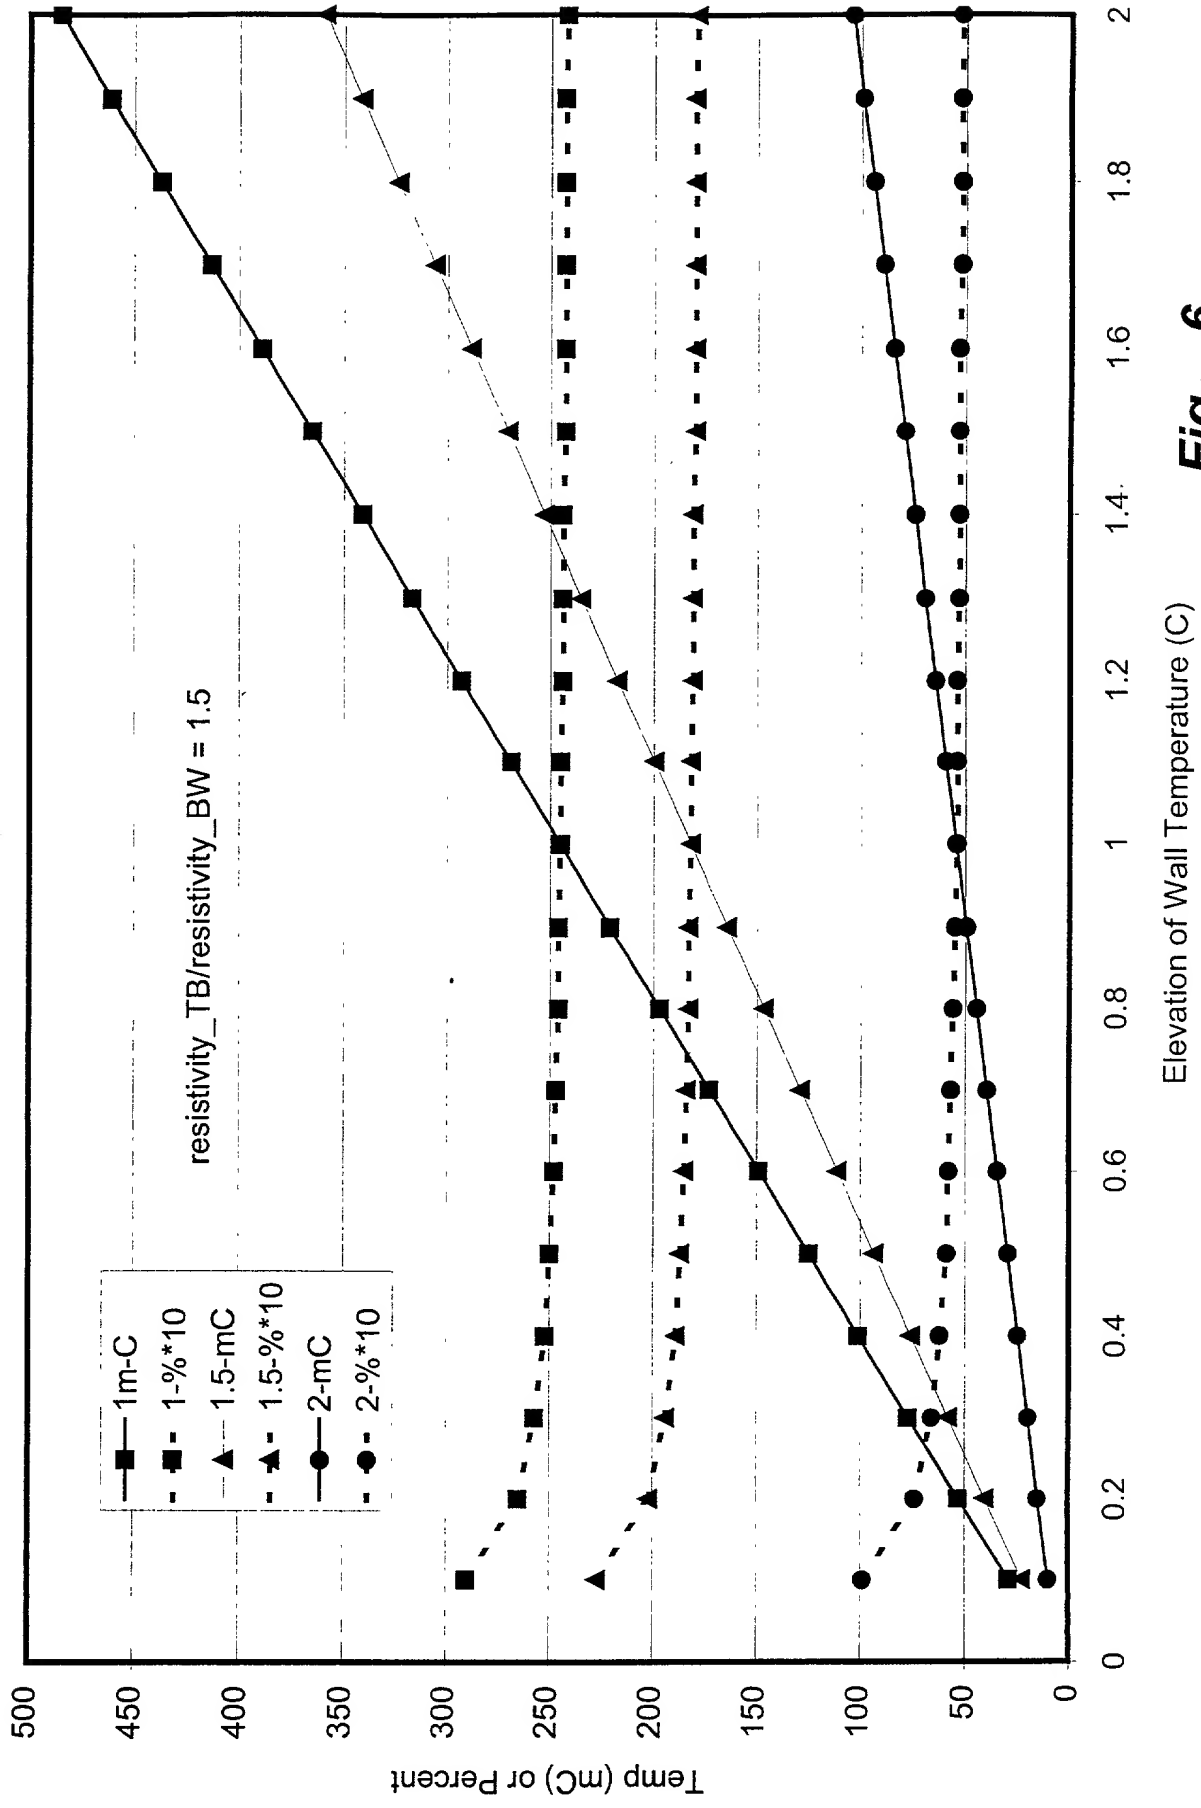


Fig - 6

# Third Sensing Arm Assymetry Experiment

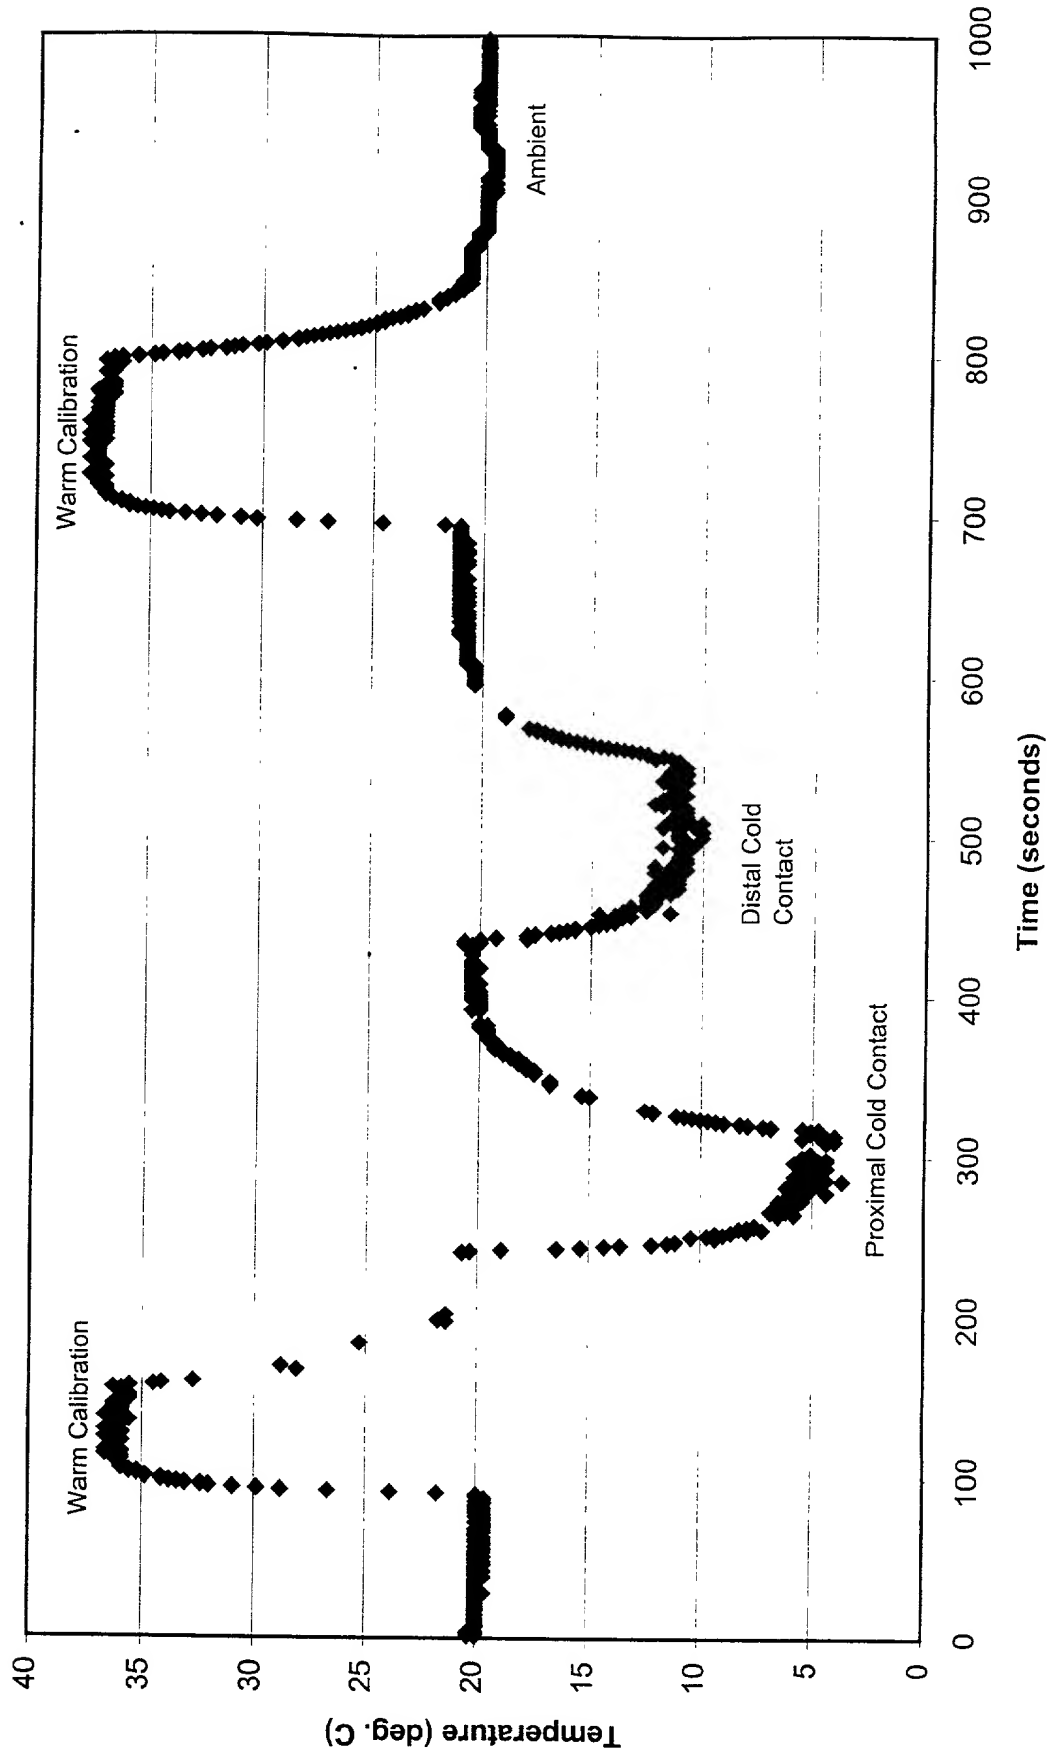


Fig - 7